

#whsterilization



video.wh.com


Now at
your dealer
or wh.com



A perfect seal in 2 seconds



seal²

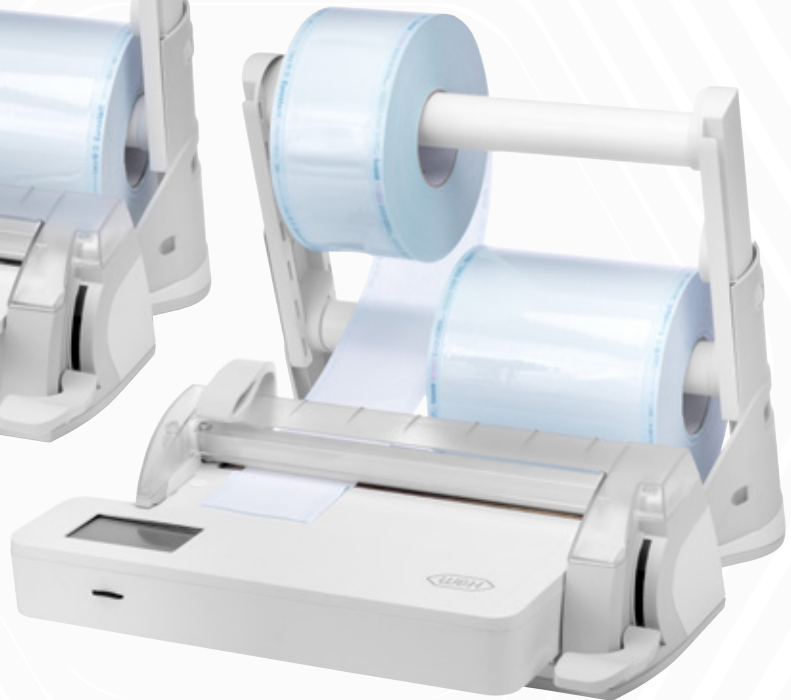

sealva!²

A **perfect** sealing process

Express packaging

It is not easy to keep a product sterile. Only an absolute hermetic and strong protection of the sterile goods against environmental influences guarantees permanent sterility.

Perfect quality seals

The foil sealer creates a 12 mm wide seal in just two seconds with no risk of burning the sterilization package.

Convenient and user-friendly

Handling is optimized with the transparent sealing unit and the integrated work surface.



Patented double-roll holder

The patented double-roll holder takes a wide range of widths.

Hermetic seal

The sealing temperature is electronically controlled and guarantees a perfect hermetic seal.

Flexible working

The roll holder can be removed from the station and mounted on the wall. This allows flexible working in the smallest spaces.

seal²

For a **validated** sealing process

Safe and secure packaging

With SeaVal², thermal sealing is now more than just sealing. The device monitors, saves and displays the data and results of the sealing process for validation. The thermal sealing and cutting of rolls and sterilization packages of laminated paper/polypropylene or other thermo-sealable material can be done easily and secure.

Full traceability

The recording of sealing parameters as pressure, time, temperature and the identification of the batch sealing responsible user ensures full traceability.

Flexible installation

The roll holder can be removed from the station and mounted on the wall. This allows flexible working in the smallest spaces.

User-friendly touchscreen


The touch screen and the intuitive menu structure facilitate the working process.

Save data

The foil sealer generates reports that can be saved on a PC via Ethernet connection or on the SD card supplied.

Pre-set and customizable


Sealing programs are available for the individual process.

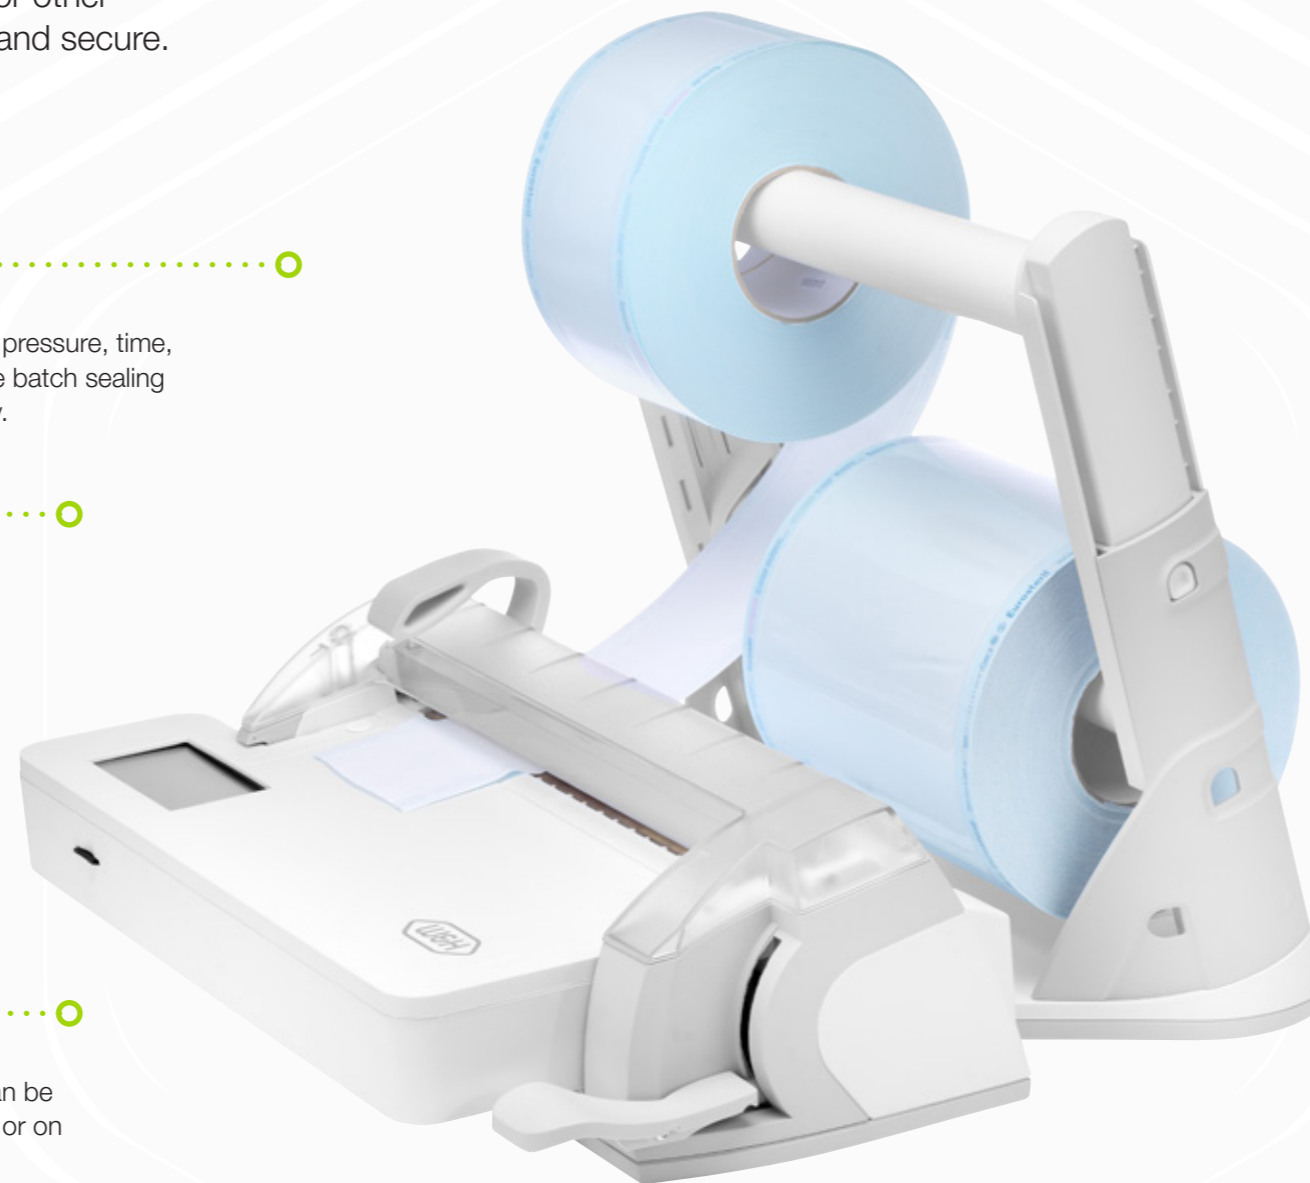

User-friendly touch screen



Flexible clamping of the rollers

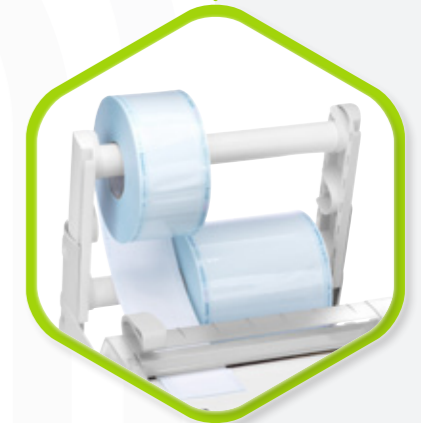

Easy lever function



sealval²

Easy checks for best results

Regular checks and verification lead to best possible results. The **Seal Check** serves exactly this purpose: verify and check the quality of the seal performed by W&H sealing devices. The routine tests support the practice to keep a high standard in the sealing process.



Seal Check

- › For validation of the closure security of sealed goods in sterilization packages.
- › Possible air leaks are monitored in order to ensure the best result in terms of sterility preservation.
- › Easy to use and integrated into the daily routine.

Technical data

Seal ²			CE
Voltage:	200/240 V AC; single phase	100/120 V AC; single phase	
Frequency:	50/60 Hz		
Power:	180 W		
Isolation class:	I/IPX0		
Fuse:	N. 2-5x 20 T4 A	N. 2-5x 20 F10 A	
Conditions of use:	Environment: Max. altitude: Temperature: Max. relative humidity: Max. voltage tolerance: Overvoltage category: Pollution degree: Max. surge (≤ 5s): Max. surge (> 5s):	Indoor use only 3000 m a.s.l. +5/+40°C 85 % ±10 % II 1 230 V + 1200 V 230 V + 250 V	
Main switch:	Bipolar		
Weight:	7.1 kg		
Welding area:	12 mm x 310 mm		
Welding temperature:	Constant		

SealVal ²			CE
Voltage:	200/240 V AC; single phase		
Frequency:	50/60 Hz		
Power:	180 W		
Isolation class:	I/IPX0		
Fuse:	Nr. 2-5x 20 T5 A		
Conditions of use:	Environment: Max. altitude: Temperature: Max. relative humidity: Max. voltage tolerance: Overvoltage category: Pollution degree: Max. surge (≤ 5s): Max. surge (> 5s):	Indoor use only 3000 m a.s.l. +5/+40°C 85 % ±10 % II 2 230 V + 1200 V 230 V + 250 V	
Main switch:	Bipolar		
Weight:	8.3 kg		
Welding area:	12 mm x 310 mm		
Welding temperature:	Standard mode Free option mode	180°C min. 170°C max. 200°C (set by the user)	

Seal² and SealVal² were designed, certified and validated with the most stringent directives and standards:

EN 868-5	Packaging for terminally sterilized medical devices – Part 5
EN 11607-2	Packaging for terminally sterilized medical devices – Part 2

W&H Sterilization Srl.
Via Bolgara, 2
24060 Brusaporto (BG), **Italy**
t +39 035-66 63 000
f +39 035-50 96 988
office.sterilization@wh.com
wh.com

W&H Dentalwerk Bürmoos GmbH
Ignaz-Glaser-Straße 53, Postfach 1
5111 Bürmoos, **Austria**
t +43 6274 6236-0
f +43 6274 6236-55
office@wh.com
wh.com